

FIG. 1

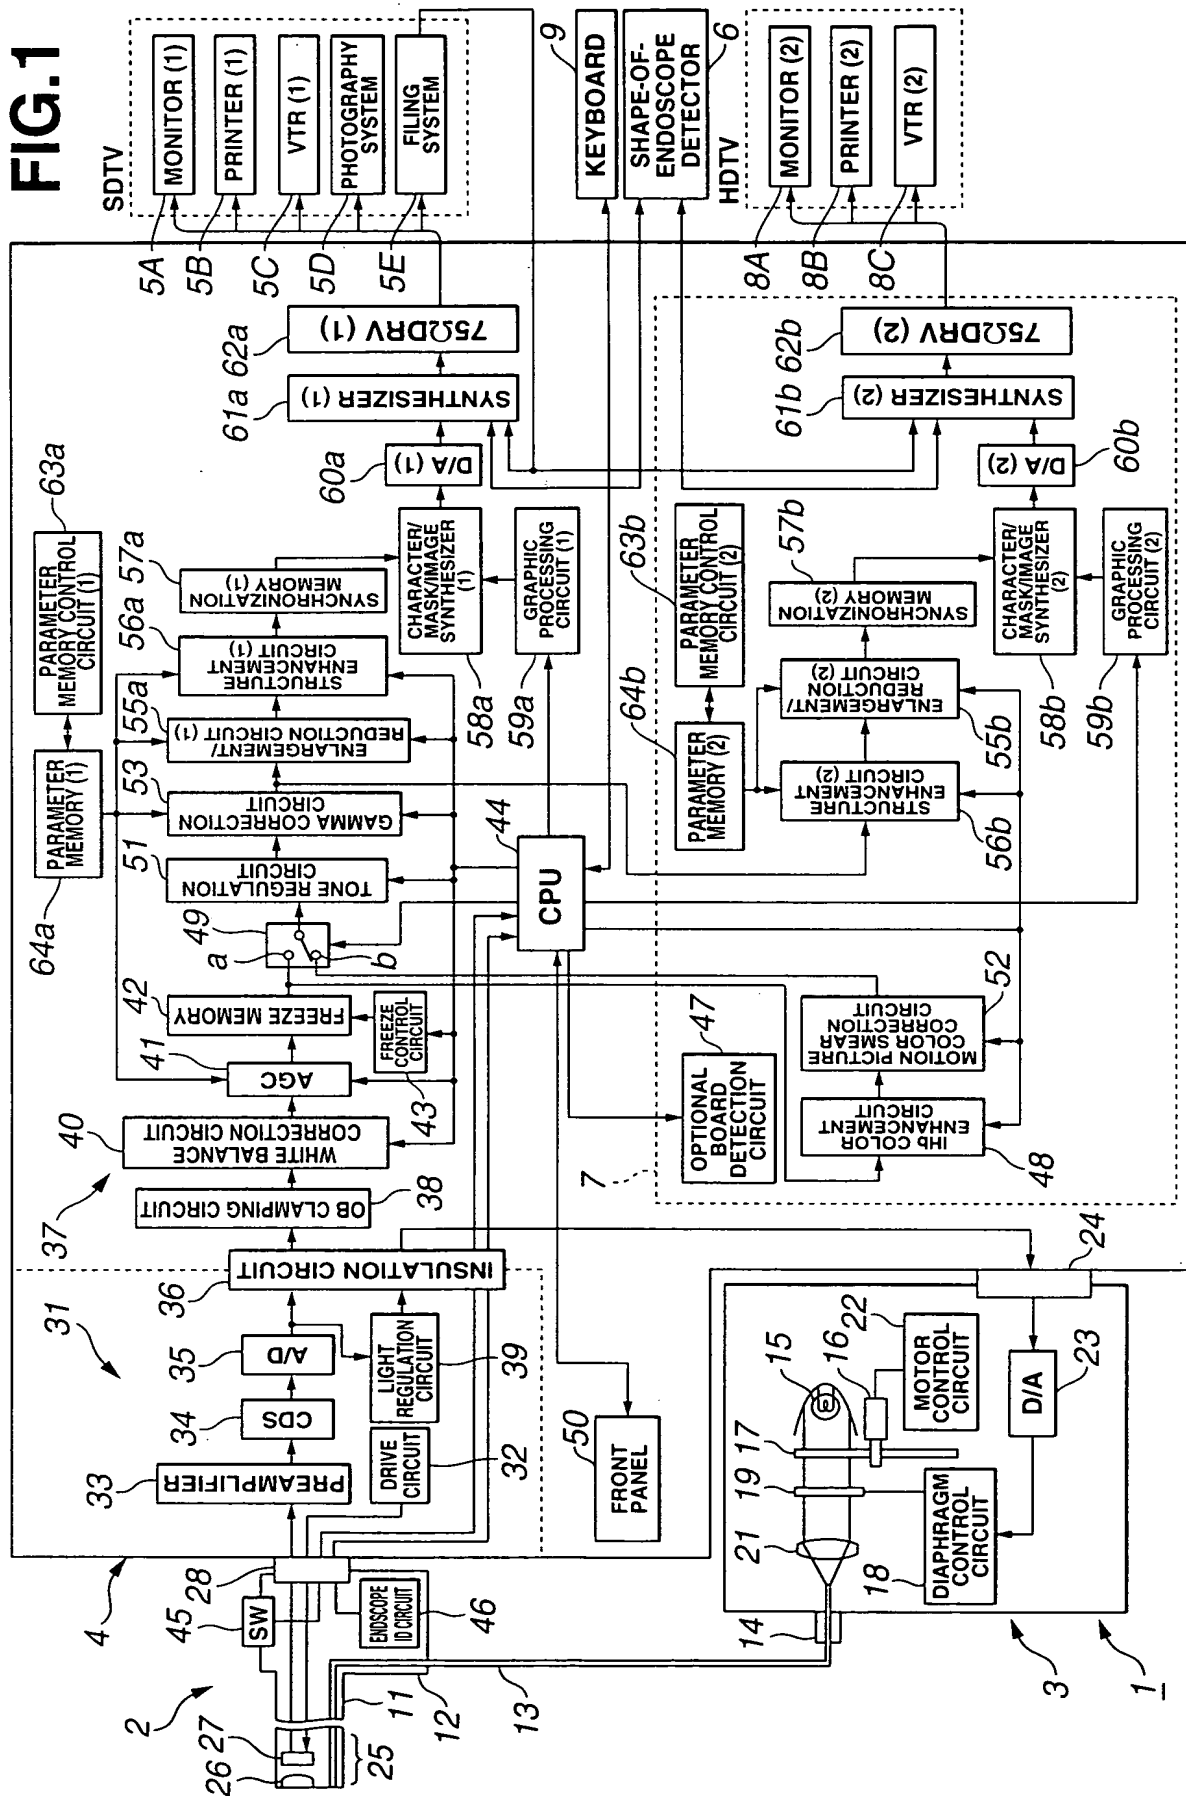
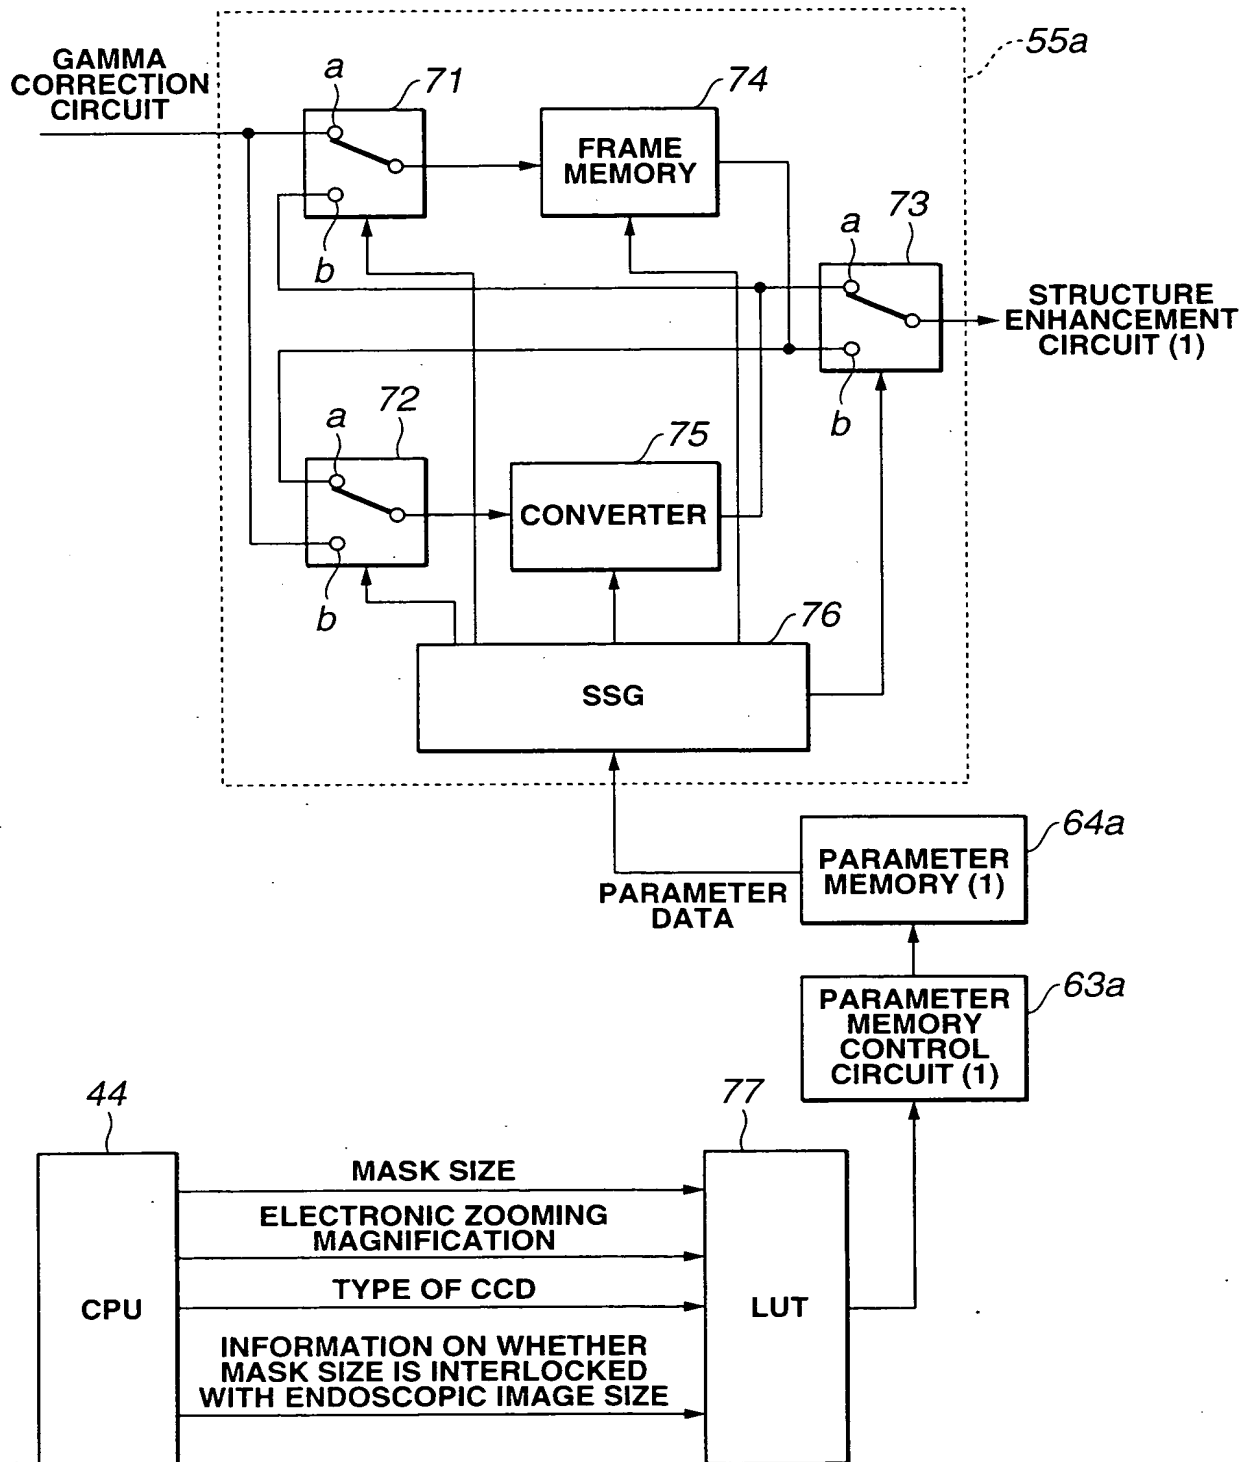


FIG. 2



SDTV

MASK SIZE	CCD	×1.0	NOT INTERLOCKED				INTERLOCKED			
			×1.4	×1.6	×1.8	×2.2	×1.4	×1.6	×1.8	×2.2
MEDIUM	TYPE1	0000h	—	—	—	—	—	—	—	—
	TYPE2	0001h	—	—	—	—	—	—	—	—
	TYPE3	0002h	0004h	0006h	0008h	000Ah	000Ch	000Eh	0010h	0012h
	TYPE4	0003h	0005h	0007h	0009h	000Bh	000Dh	000Fh	0011h	0013h
SEMI-FULL	TYPE1	—	—	—	—	—	—	—	—	—
	TYPE2	1000h	—	—	—	—	—	—	—	—
FULL-HEIGHT	TYPE3	1001h	1003h	1005h	1007h	1009h	100Bh	100Dh	100Fh	1011h
	TYPE4	1002h	1004h	1006h	1008h	100Ah	100Ch	100Eh	1010h	1012h
	TYPE1	2000h	—	—	—	—	—	—	—	—
	TYPE2	2001h	—	—	—	—	—	—	—	—
FULL-HEIGHT	TYPE3	2002h	2004h	2006h	2008h	200Ah	—	—	—	—
	TYPE4	2003h	2005h	2007h	2009h	200Bh	—	—	—	—

FIG.3A

HDTV

MASK SIZE	CCD	×1.0	NOT INTERLOCKED				INTERLOCKED			
			×1.4	×1.6	×1.8	×2.2	×1.4	×1.6	×1.8	×2.2
MEDIUM	TYPE1	0000h	—	—	—	—	—	—	—	—
	TYPE2	0001h	—	—	—	—	—	—	—	—
	TYPE3	0002h	0004h	0006h	0008h	000Ah	000Ch	000Eh	0010h	0012h
	TYPE4	0003h	0005h	0007h	0009h	000Bh	000Dh	000Fh	0011h	0013h
SEMI-FULL	TYPE1	1000h	—	—	—	—	—	—	—	—
	TYPE2	1001h	—	—	—	—	—	—	—	—
FULL-HEIGHT	TYPE3	1002h	1004h	1006h	1008h	100Ah	100Ch	100Eh	1010h	1012h
	TYPE4	1003h	1005h	1007h	1009h	100Bh	100Dh	100Fh	1011h	1013h
	TYPE1	2000h	—	—	—	—	—	—	—	—
	TYPE2	2001h	—	—	—	—	—	—	—	—
FULL-HEIGHT	TYPE3	2002h	2004h	2006h	2008h	200Ah	—	—	—	—
	TYPE4	2003h	2005h	2007h	2009h	200Bh	—	—	—	—

FIG.3B

FIG.4A

(MEDIUM)

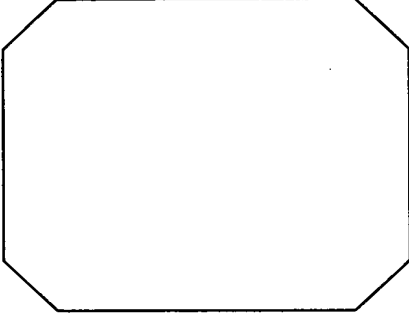
ID No. : Sex:Age: D.O.Birth 2001/04/01 23:59:59 SCV:1 CVP:A1/4 D.F:99 VTR Ct:NEH:A3 Ce:1Z:1.0	Name: 
Physician: Comment:	

FIG.4B

(SEMI-FULL)

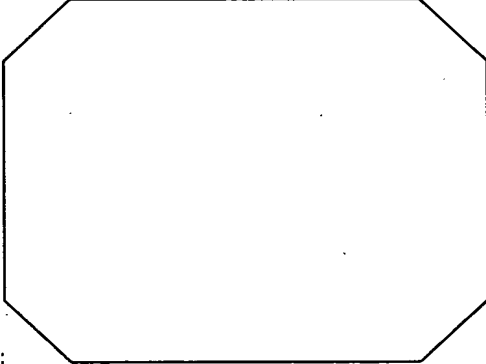
ID No. : Name: Name: Sex:Age: D.O.Birth 2001/04/01 23:59:59 SCV:1 CVP:A1/4 D.F:99 VTR Ct:NEH:A3 Ce:1Z:1.0	
Physician: Comment:	

FIG.4C

(FULL-HEIGHT)

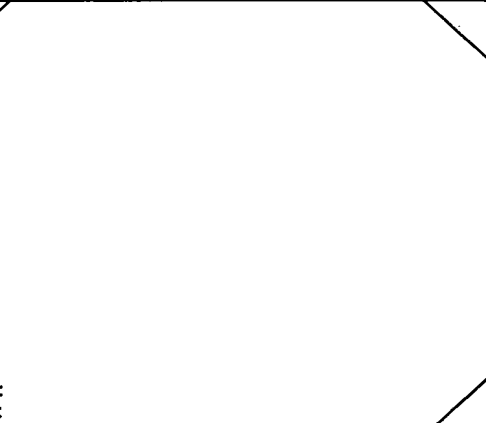
ID No. : Name: Name: Sex:Age: D.O.Birth 2001/04/01 23:59:59 SCV:1 CVP:A1/4 D.F:99 VTR Ct:NEH:A3 Ce:1Z:1.0	
Physician: Comment:	

FIG.5A

(Z=1. 0)

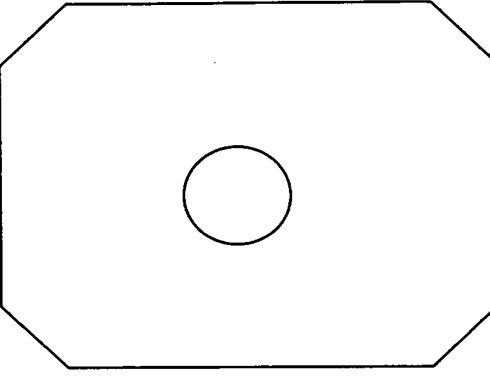
ID No. :	
Name:	
Sex:Age:	
D.O.Birth	
2001/04/01 23:59:59	
SCV:1	
CVP:A1/4	
D.F:99	
VTR	
Ct:NEH:A3	
Ce:1Z:1.0	
Physician:	
Comment:	

FIG.5B

(Z=1. 6)

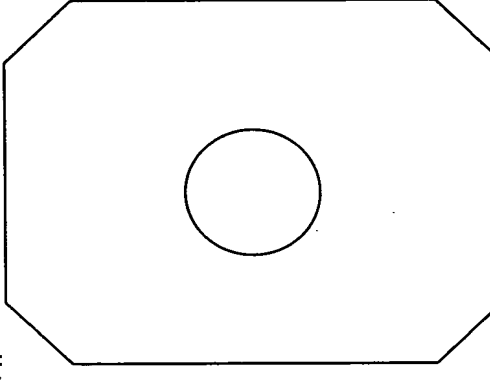
ID No. :	
Name:	
Sex:Age:	
D.O.Birth	
2001/04/01 23:59:59	
SCV:1	
CVP:A1/4	
D.F:99	
VTR	
Ct:NEH:A3	
Ce:1Z:1.6	
Physician:	
Comment:	

FIG.5C

(Z=2. 2)

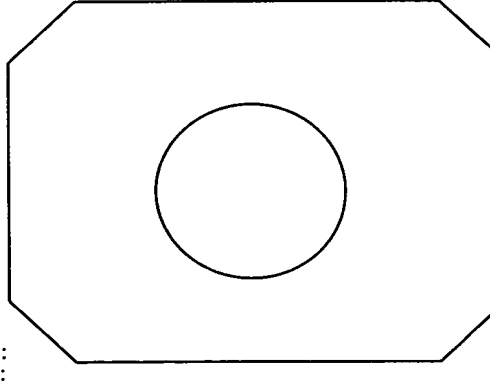
ID No. :	
Name:	
Sex:Age:	
D.O.Birth	
2001/04/01 23:59:59	
SCV:1	
CVP:A1/4	
D.F:99	
VTR	
Ct:NEH:A3	
Ce:1Z:2.2	
Physician:	
Comment:	

FIG.6

Endoscope switch Switch 1: Freeze Switch 2: Enhance Switch 3: Printer Switch 4: Release			Photometry Average IHb IHb area : All IHb range : Normal IHb average value : Off Enlargement Level 1 : 1.6 Level 2 : 2.2 Changing sizes : Off		
Enhancement Mode 1: A1 Mode 2: A3 Mode 3: A5	Structure enhancement A1 A3 A5	Color enhancement 0 3 5	Mask size SD Semi-full← →Full height HD Semi-full← →Full height		
Type of enhancement : structure Handling for enhancement : independent			Reset		

Press ↑ and ↓ buttons to change items,
and press ← and → buttons for changing settings.
Press Enter buttons to save data and complete entry.
press Esc button to terminate menu selection.

FIG.7

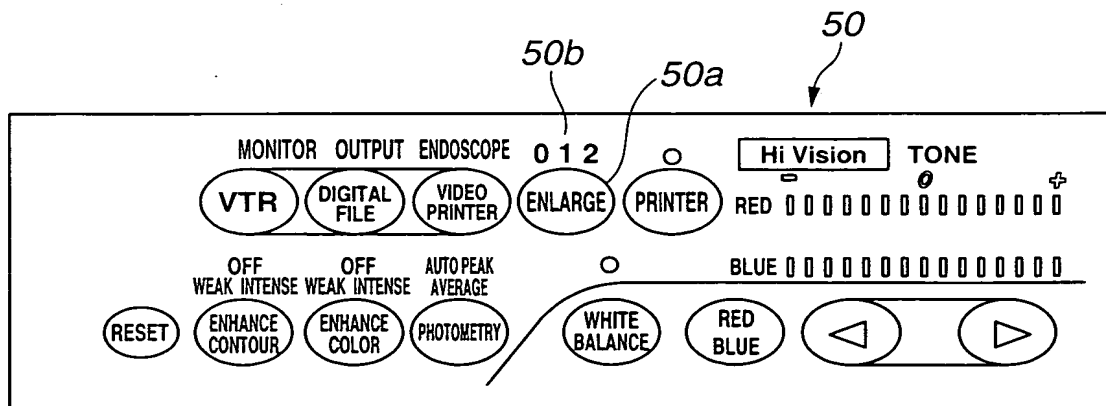


FIG.8A

(Z=1. 0)

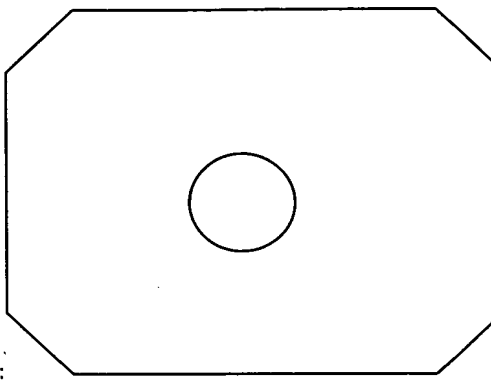
ID No. :	
Name:	
Sex:Age:	
D.O.Birth	
2001/04/01	
23:59:59	
SCV:1	
CVP:A1/4	
D.F:99	
VTR	
Ct:NEH:A3	
Ce:1Z:1.0	
Physician:	
Comment:	

FIG.8B

(Z=1. 6)

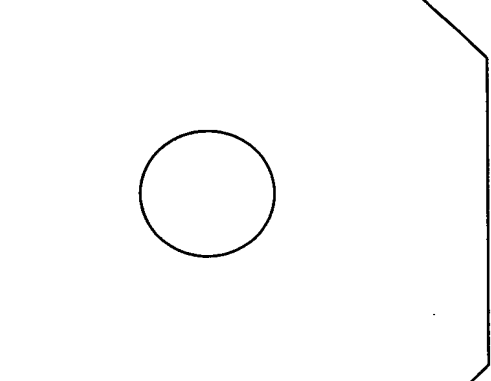
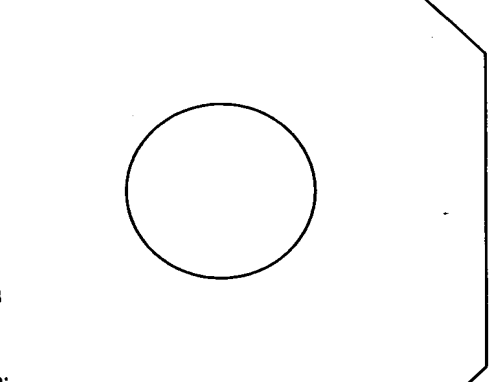
ID No. :	
Name:	
Sex:Age:	
D.O.Birth	
2001/04/01	
23:59:59	
SCV:1	
CVP:A1/4	
D.F:99	
VTR	
Ct:NEH:A3	
Ce:1Z:1.5	
Physician:	
Comment:	

FIG.8C

(Z=2. 2)

ID No. :	
Name:	
Sex:Age:	
D.O.Birth	
2001/04/01	
23:59:59	
SCV:1	
CVP:A1/4	
D.F:99	
VTR	
Ct:NEH:A3	
Ce:1Z:2.2	
Physician:	
Comment:	

10/501695

FIG.9

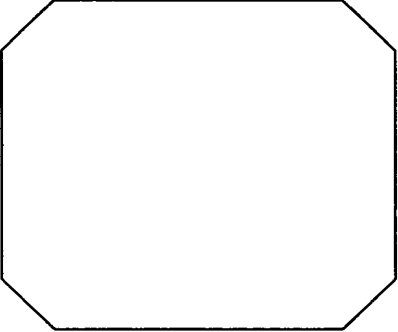
ID No. : Sex:Age: D.O.Birth	Name:
2001/04/01 23:59:59	
SCV:1 CVP:A1/4 D.F:99 VTR	
CT:NEH:A3 CE:1	
Physician:	
Comment:	

FIG.10

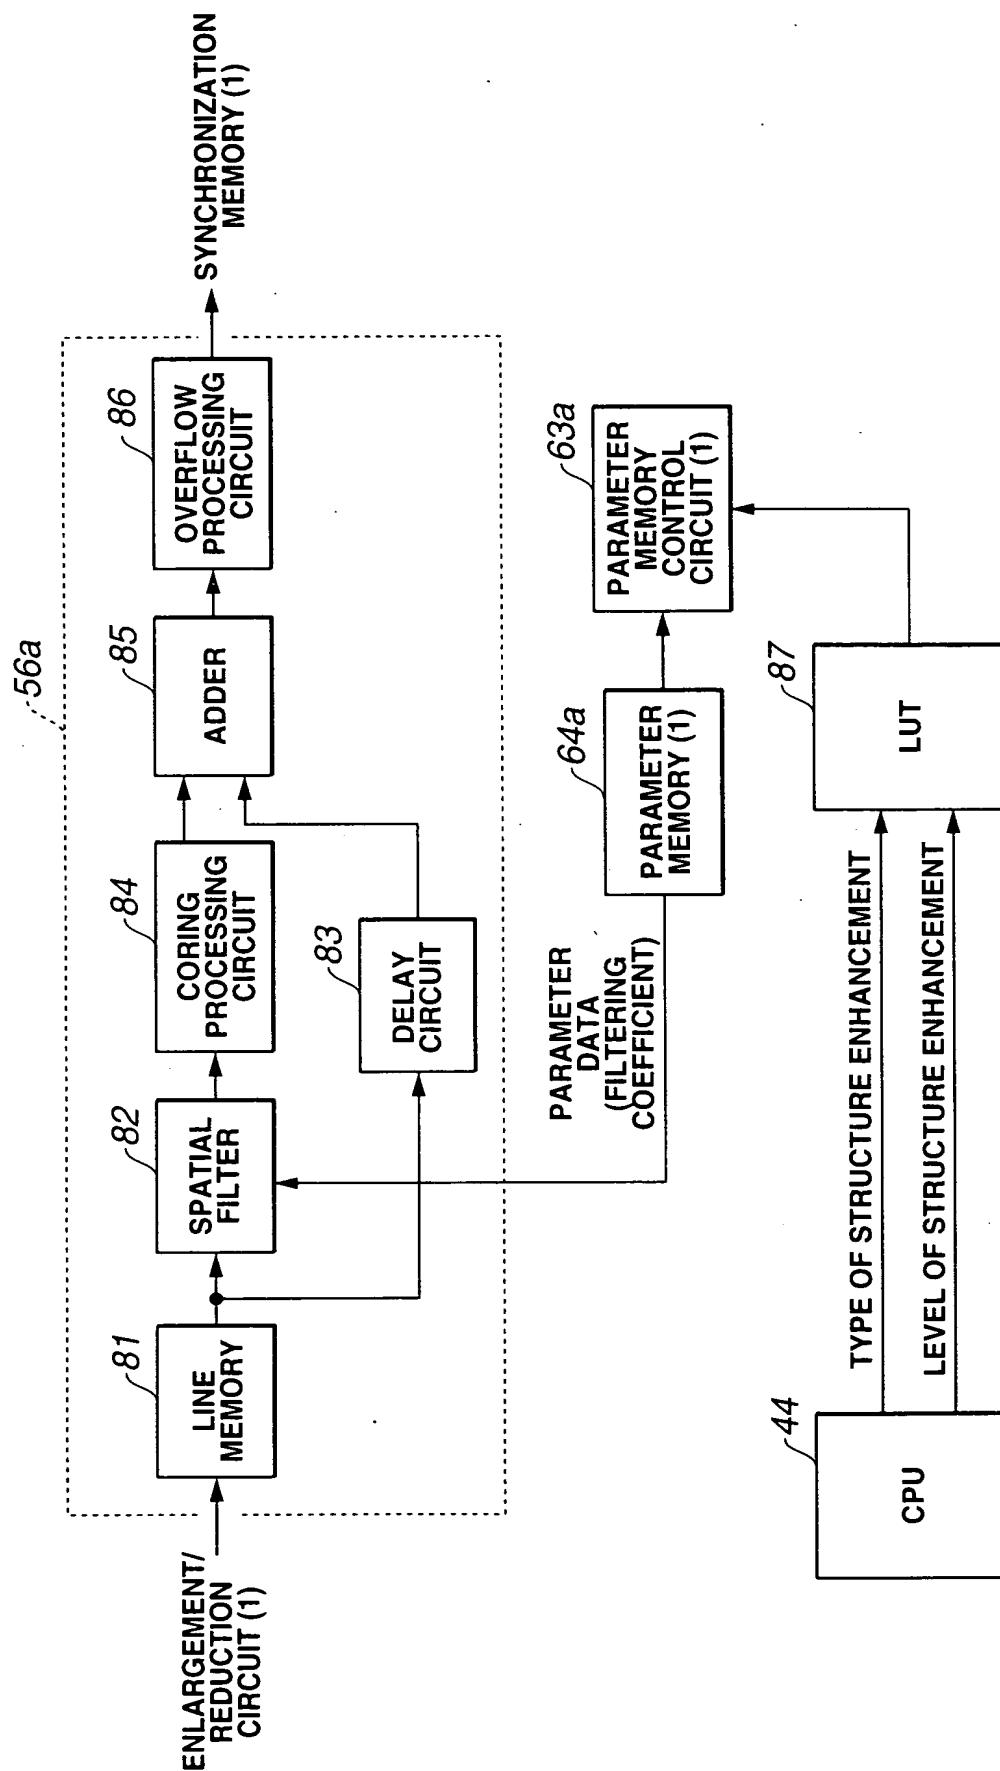


FIG.11

ID No. : Sex:Age: D.O.Birth	Name:	
2001/04/01 23:59:59	ELECTRONIC ENDOSCOPIC IMAGE	
SCV:1 CVP:A1/4 D.F:99 VTR		
Ct:NEH:A3 Ce:1 Z:1:1.0		
IMAGE PRODUCED BY SHAPE-OF- ENDSCOPE DETECTOR		

FIG.15A

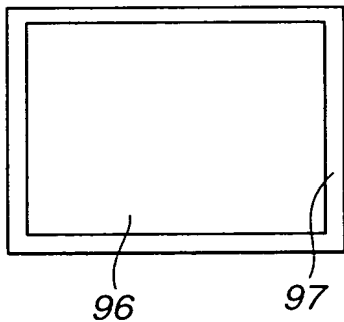


FIG.15B

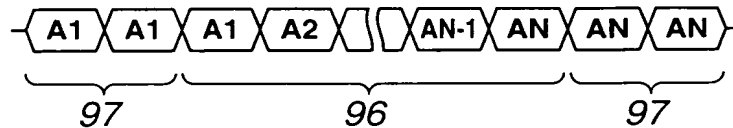


FIG.12

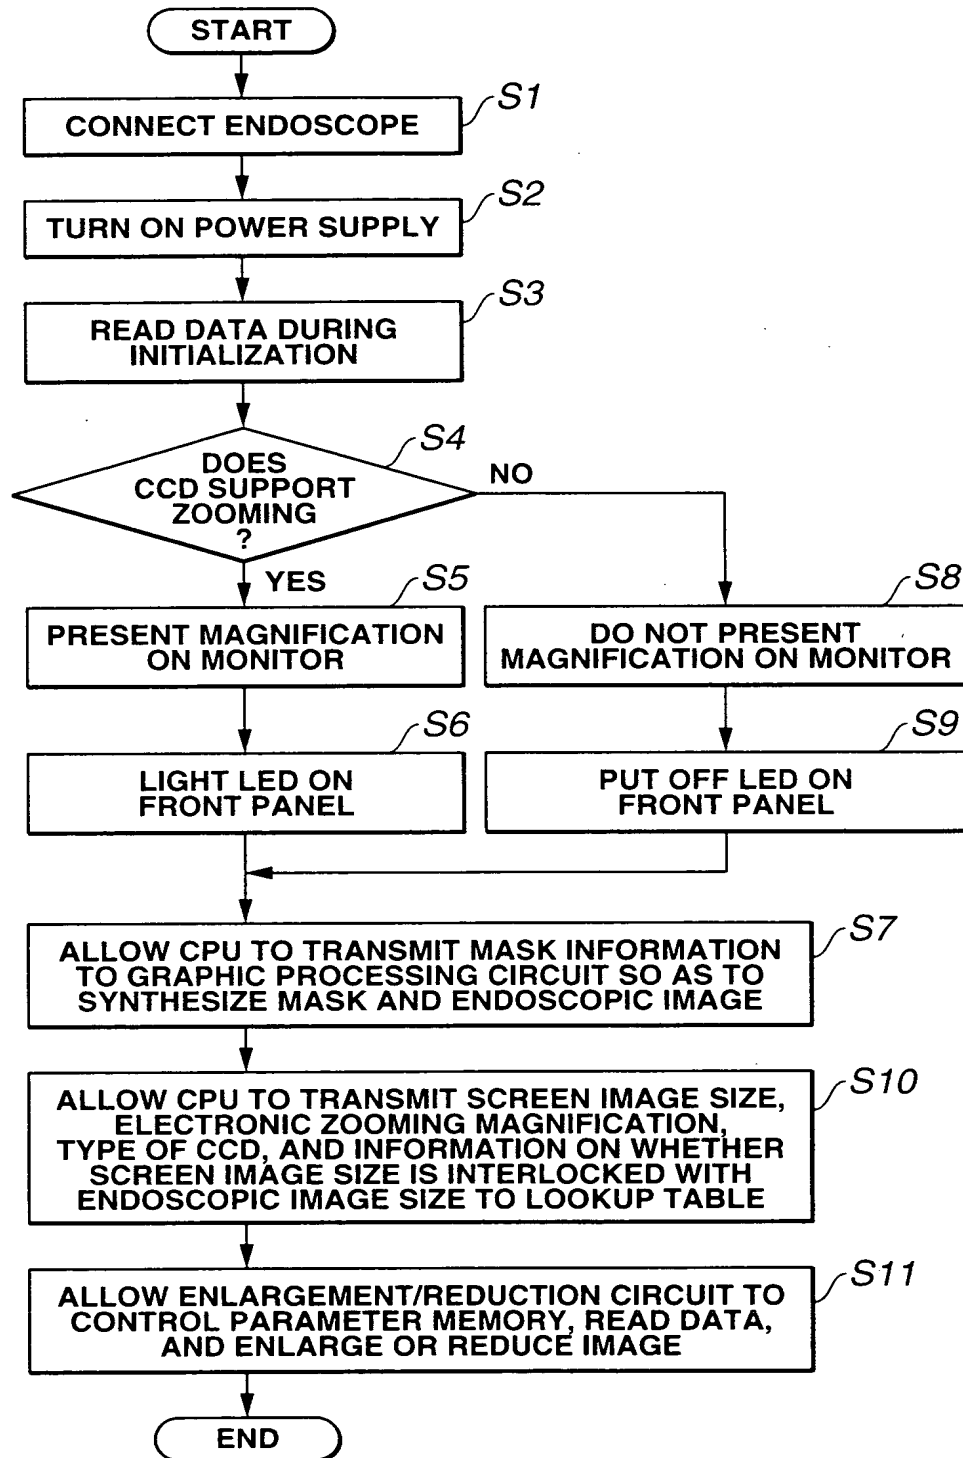


FIG.13

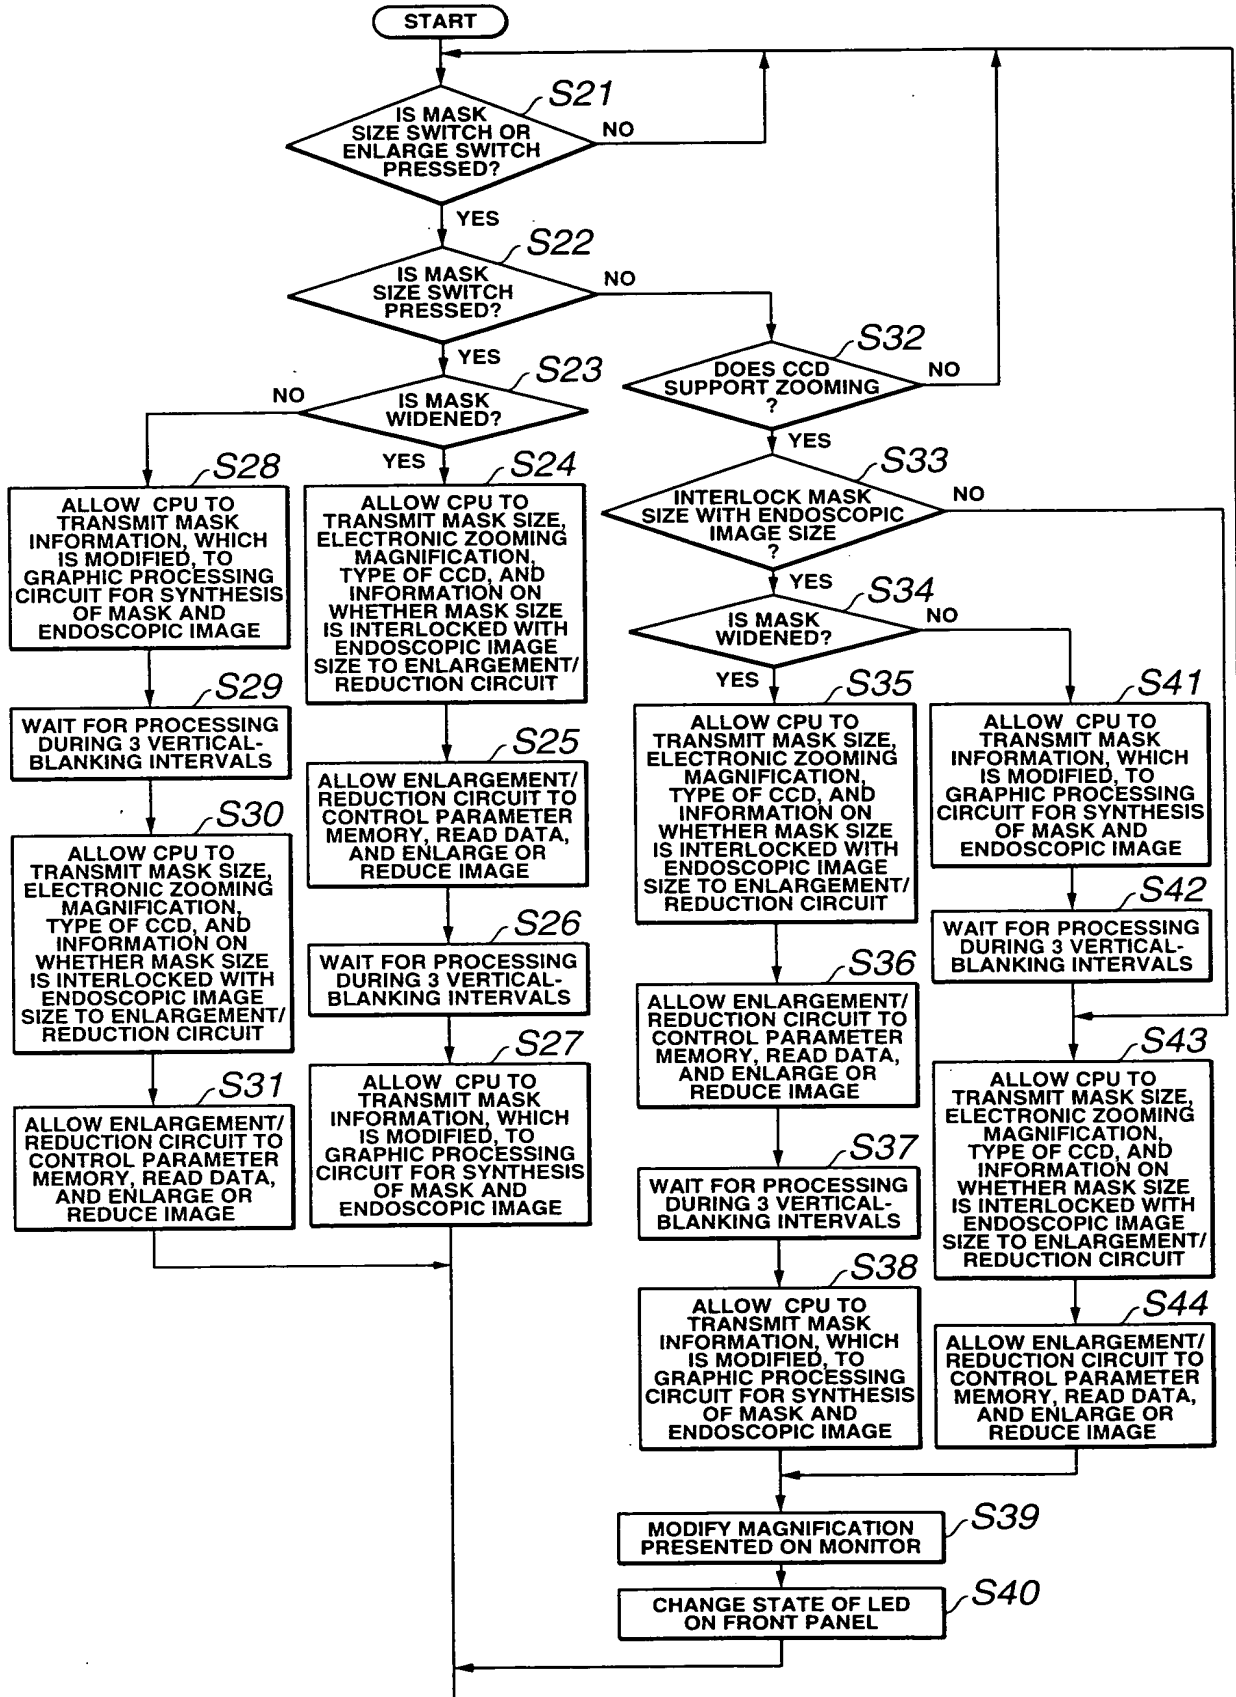


FIG. 14

